

Applicant(s): C. Desylva et al.
INSTRUCTION MIX MONITOR

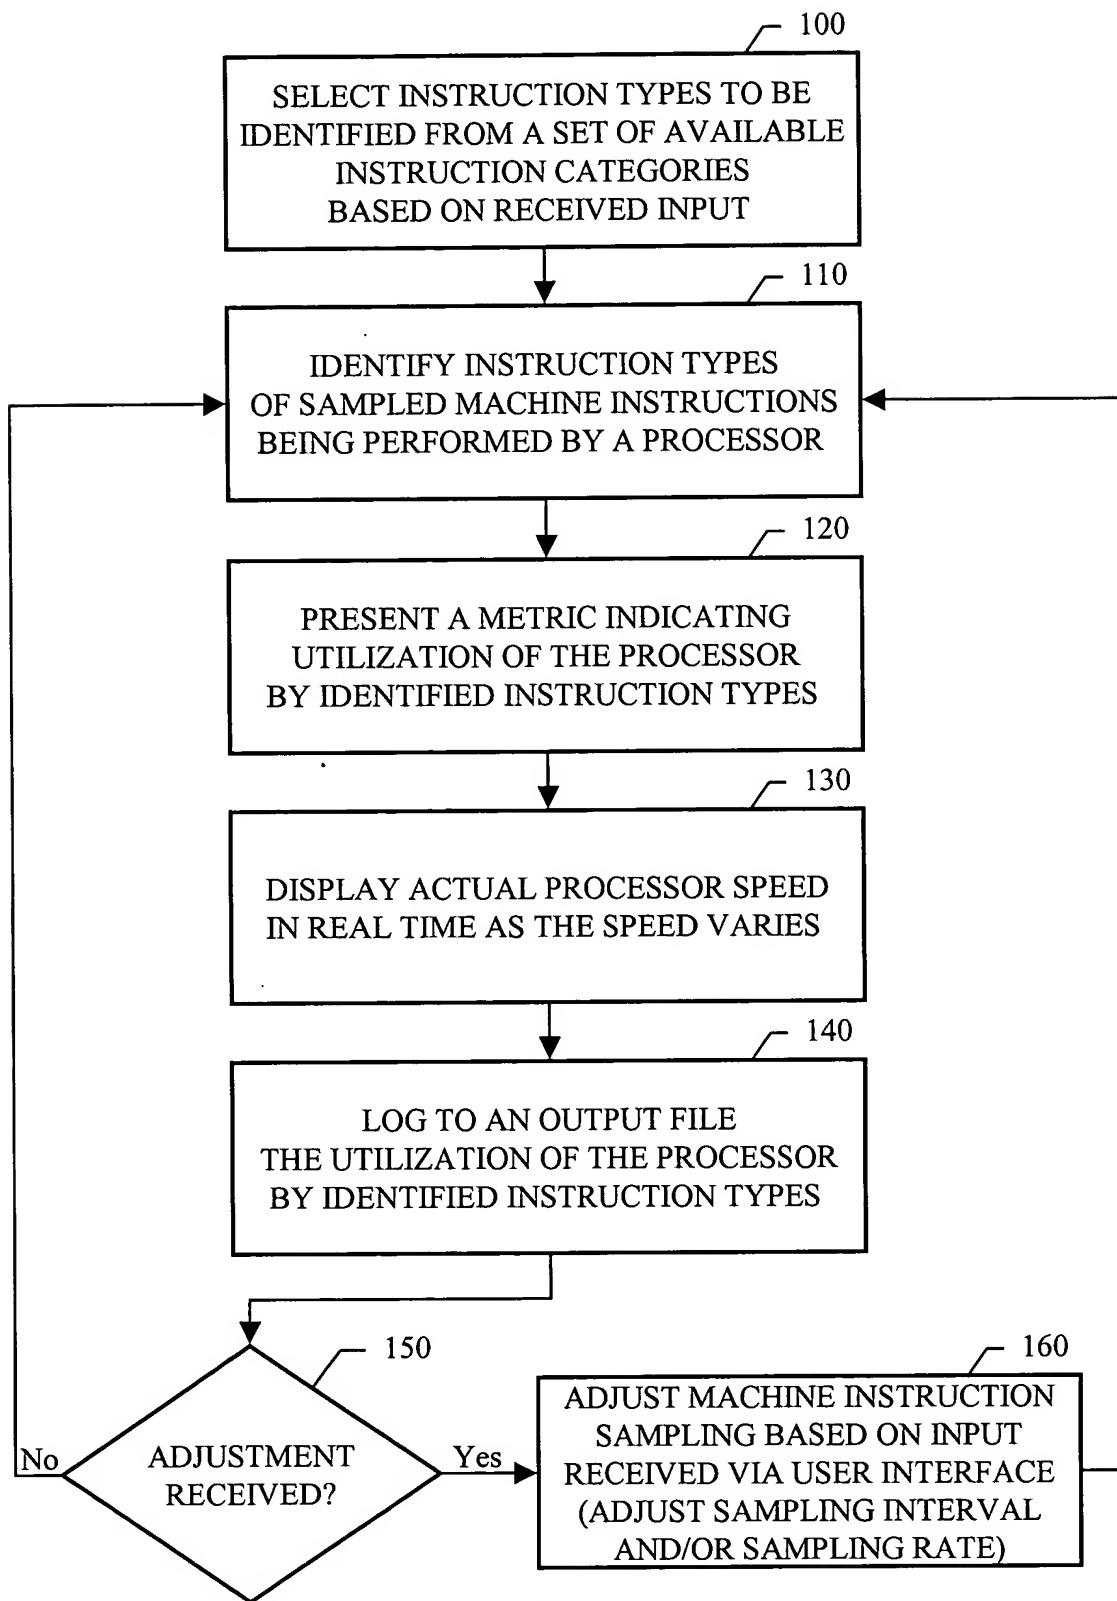


FIG. 1





Applicant(s): C. Desylva et al.
INSTRUCTION MIX MONITOR

FIG. 2

Applicant(s): C. Desylva et al.
INSTRUCTION MIX MONITOR

**FIG. 3**

Applicant(s): C. Desylva et al.
INSTRUCTION MIX MONITOR

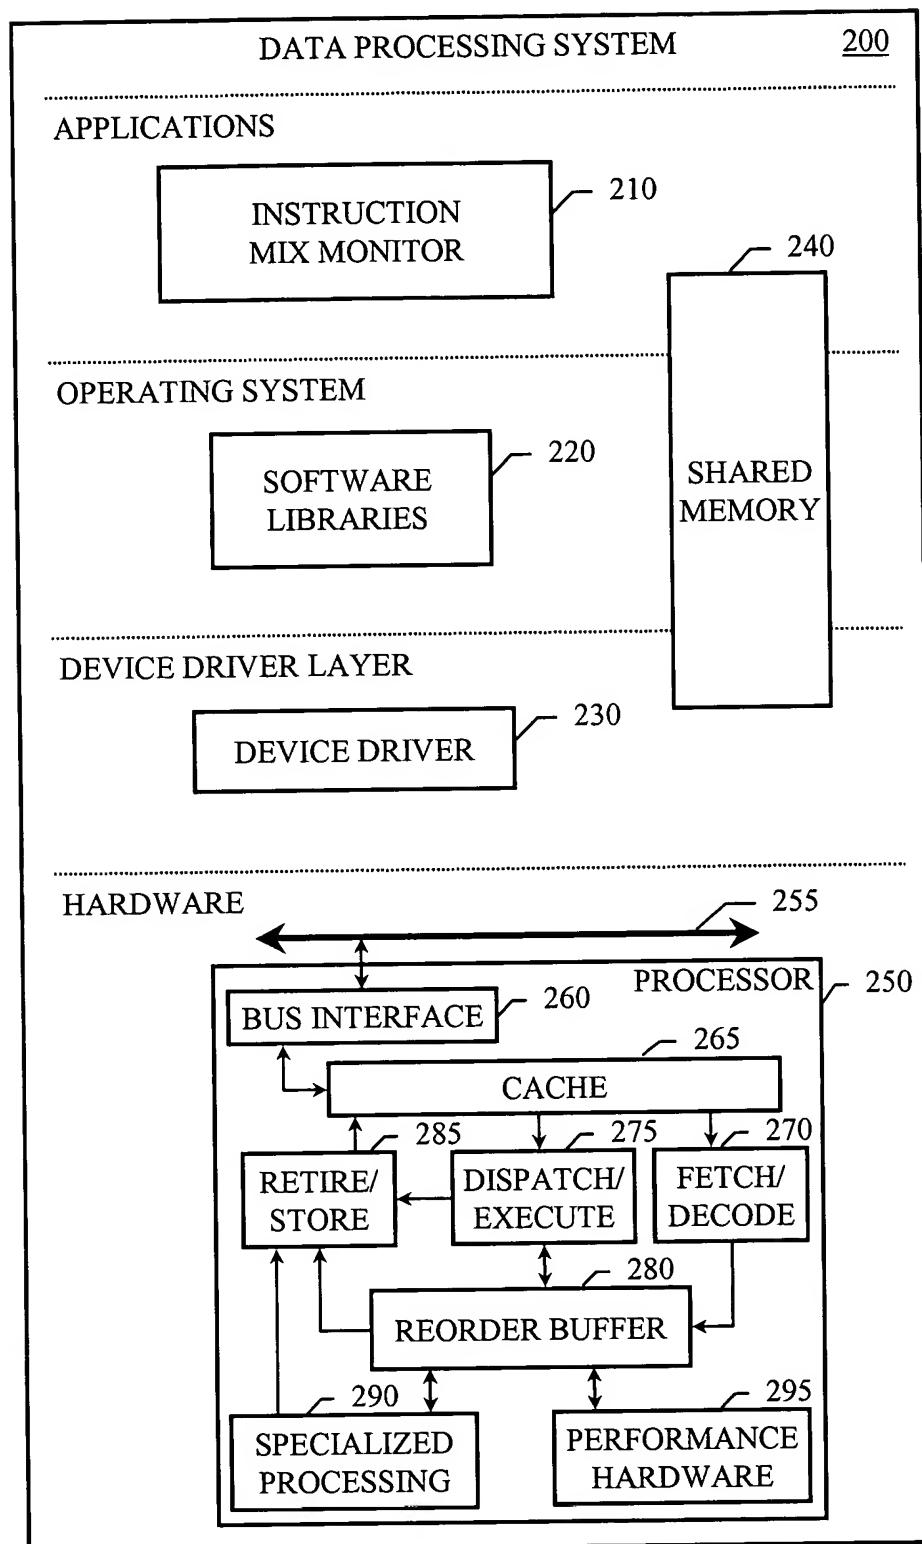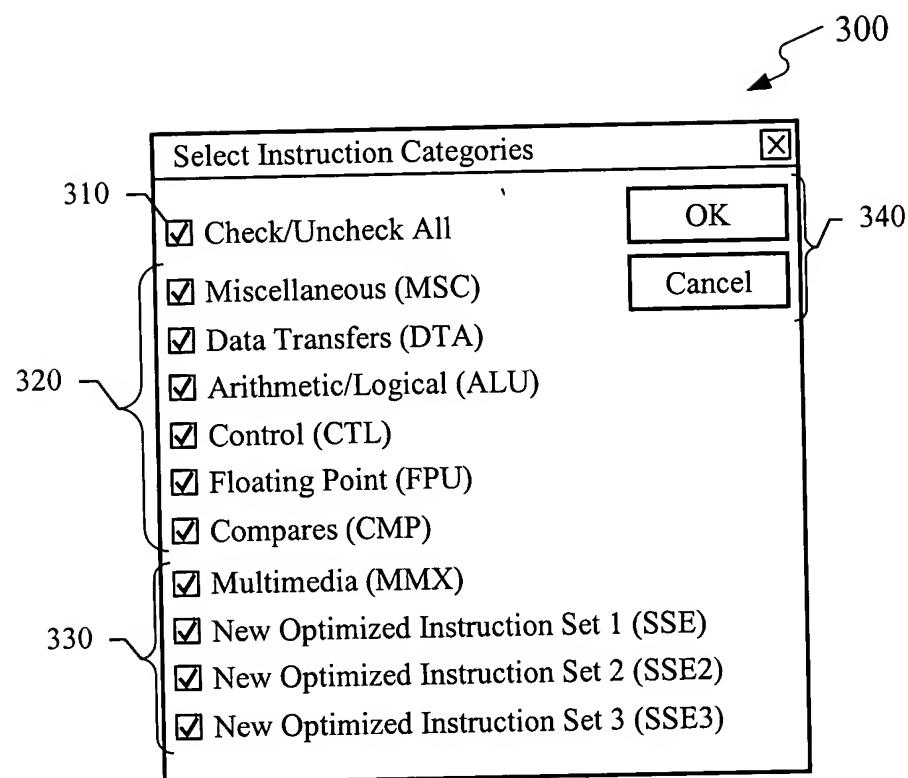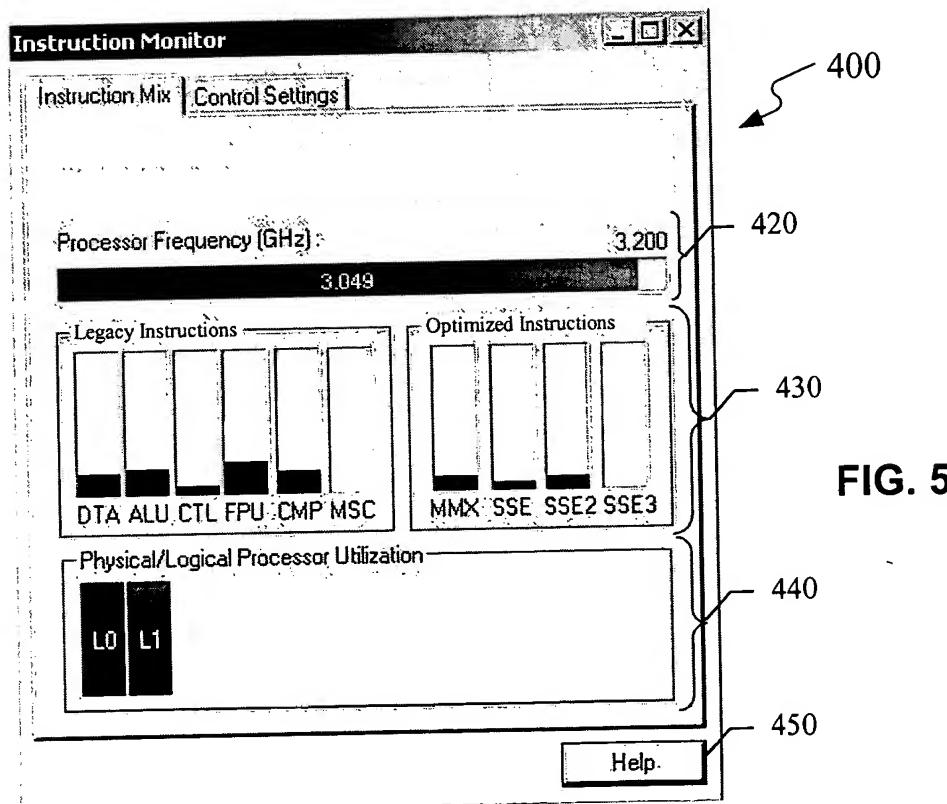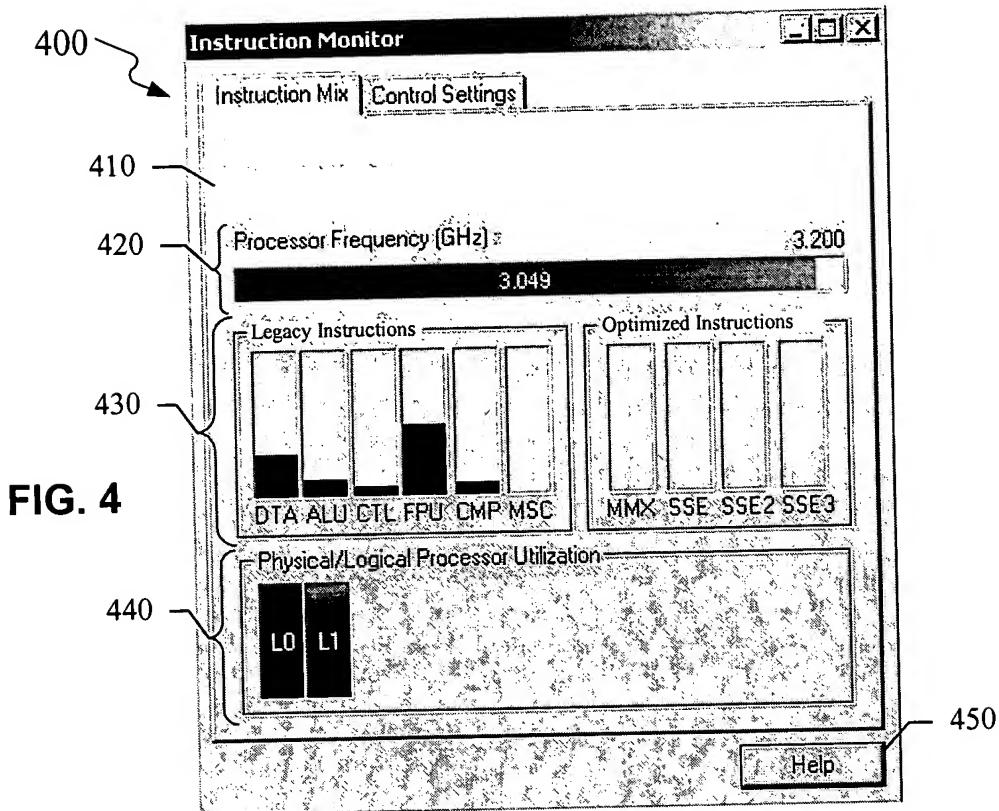

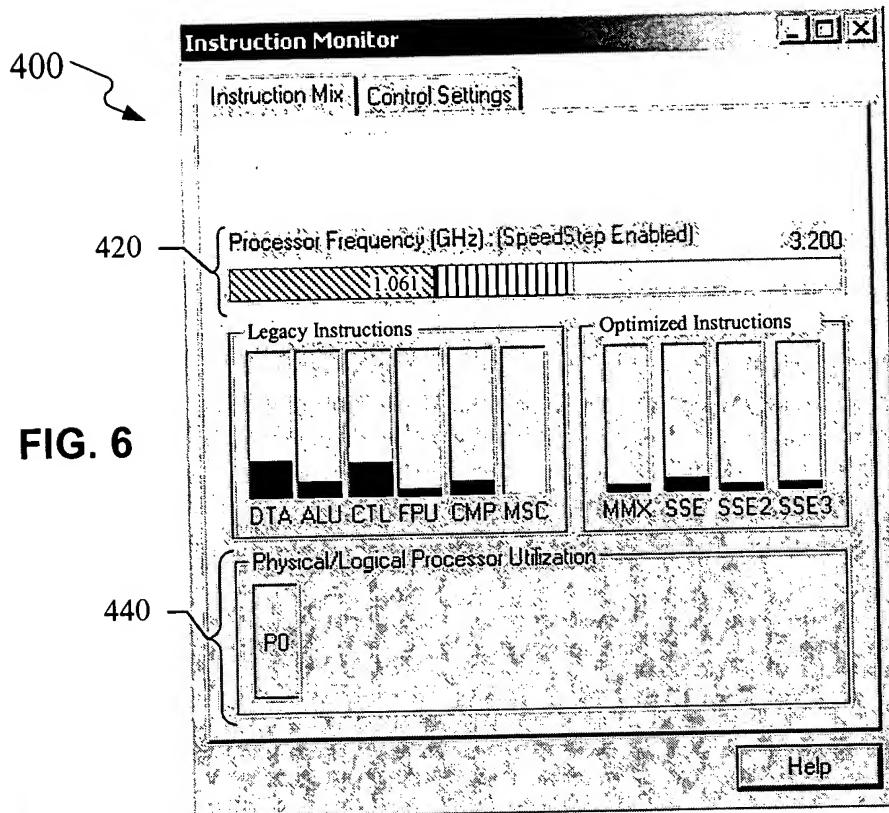
Applicant(s): C. Desylva et al.
INSTRUCTION MIX MONITOR

FIG. 6

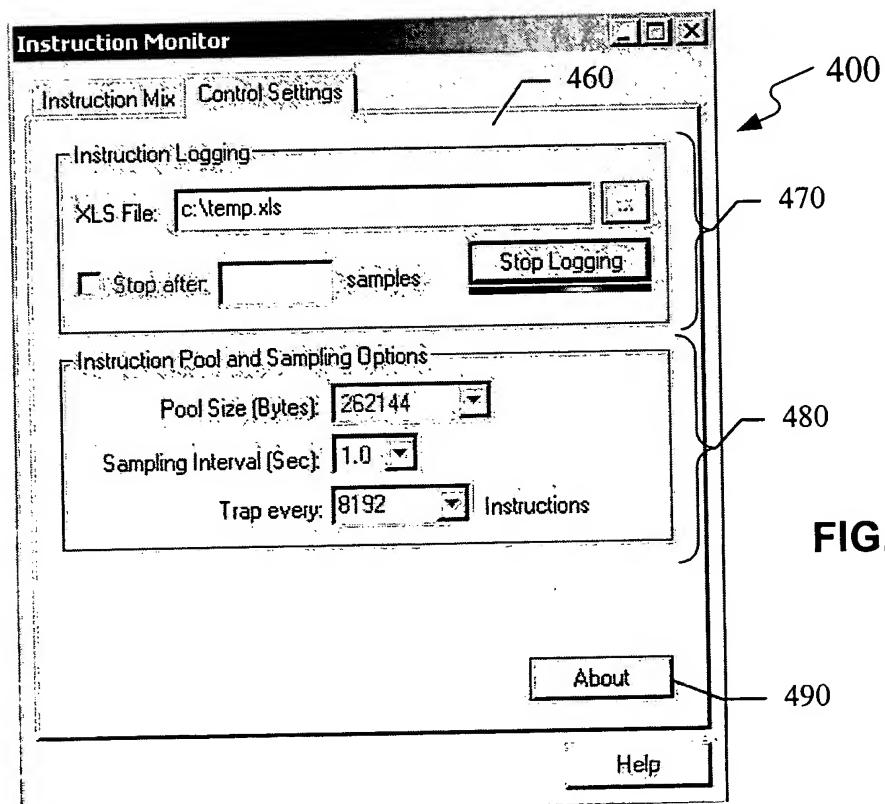


FIG. 7